



PicoScope 6000 Series PC Oscilloscopes

User's Guide



Contents


1 Welcome	1
2 Introduction	2
1 Using this guide	2
2 Safety symbols	2
3 Safety warnings	2
4 FCC notice	3
5 CE notice	3
6 Software licence conditions	4
7 Trademarks	5
8 Warranty	5
9 Company details	5
3 Product information	6
1 Package contents	6
2 Minimum PC requirements	6
3 Installation instructions	7
4 Connections	8
5 Specifications	9
4 Glossary	11
Index.....	13



1 Welcome

Thank you for buying a PicoScope 6000 Series oscilloscope from Pico Technology!

The PicoScope 6000 Series scopes have comparable features and specifications to traditional bench-top oscilloscopes, but are more economical and take up only a fraction of the space.

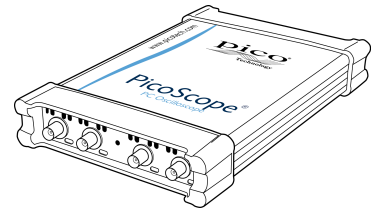


Here are some of the benefits provided by your new PicoScope 6000 Series oscilloscope:

- **Portability:** Take the unit with you and plug it in to any Windows PC.
- **Performance:** Up to 5 GS/s sampling, 500 MHz bandwidth and 1 **GS** ¹¹¹ buffer.
- **Flexibility:** Use it as an oscilloscope, spectrum analyzer or high-speed data acquisition interface.
- **Programmability:** The PicoScope 6000 Series SDK lets you write your own programs, in your chosen programming language, to control all the features of the scope.
- **Long-term support:** Software upgrades are available to download from our [website](#). You can also call our technical specialists for support. You can continue to use both of these services free of charge for the lifetime of the product.
- **Value for money:** You don't have to pay twice for all the features that you already have in your PC, as the PicoScope 6000 Series scope contains the special hardware you need and nothing more.
- **Convenience:** The software makes full use of the full-sized display, disk storage, user interface and networking built in to your PC.
- **Five-year warranty:** Your oscilloscope is covered for five years from the day of purchase against manufacturing faults. We don't charge a penny extra for this benefit.

2 Introduction

2.1 Using this guide

You will sometimes see a symbol like this:  This is the cross-reference symbol, and it indicates the number of a page on which you can find more information about a topic.

2.2 Safety symbols

The following symbols appear on the front panel of the PicoScope 6000 Series oscilloscope.

Symbol 1: Warning triangle



This symbol indicates that a safety hazard exists on the indicated connections if correct precautions are not taken. Read all safety documentation associated with the product before using it.

Symbol 2: Equipotential



This symbol indicates that the outer shells of the indicated BNC connectors are all at the same potential (shorted together). You must therefore take necessary precautions to avoid applying a potential across the return connections of the indicated BNC terminals. Such a potential could cause a large current to flow, resulting in damage to the product or connected equipment, or both.

2.3 Safety warnings



We strongly recommend that you read the general safety information below before using your oscilloscope for the first time. Safety protection built in to equipment may cease to function if the equipment is used incorrectly. This could cause damage to your computer, or lead to injury to yourself and others.

DO NOT exceed the overload protection range. The product is designed to measure signals within the ranges stated in the "Voltage ranges" section of the [Specifications table](#)^[9]. The inputs can withstand the wider range of voltages stated in the "Overload protection" section of the [same table](#)^[9]. Contact with voltages outside the overload protection range may cause permanent damage to the unit.

DO NOT connect to mains voltages. The product is not designed for use with mains voltages (also known as line voltages, or house current). To measure mains voltages, use a differential isolating probe specifically rated for mains use.

DO NOT rely on the scope's ground as a safety ground. The product connects directly to the ground of a computer through the USB cable provided. This ground is for signalling and shielding, and is not a safety ground.

DO NOT connect the ground input to any potential other than ground. If in doubt, use a meter to check that there is no significant AC or DC voltage between the ground input of the oscilloscope and the point to which you intend to connect it. Connecting the ground input to a voltage source may cause damage to the scope and the computer, and injury to yourself and others.

2.4 FCC notice

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his or her own expense.

For safety and maintenance information see the [safety warning](#)^[2].

2.5 CE notice

The product meets the intent of the EMC directive 89/336/EEC and has been tested to EN61326-1:2006 Class A Emissions and Immunity standard.

The product also meets the intent of the Low Voltage Directive and has been designed to meet the BS EN 61010-1:2010 IEC 61010-1:2010 Safety requirements for electrical equipment for measurement, control, and laboratory use standard.

2.6 Software licence conditions

The material contained in this software release is licensed, not sold. Pico Technology Limited grants a licence to the person who installs this software, subject to the conditions listed below.

Access. The licensee agrees to allow access to this software only to persons who have been informed of these conditions and agree to abide by them.

Usage. The software in this release is for use only with Pico Technology products or with data collected using Pico Technology products.

Copyright. Pico Technology Ltd. claims the copyright of, and retains the rights to, all material (software, documents etc.) contained in this release. You may copy and distribute the PicoScope and PicoLog software and drivers with no modifications, additions or omissions. You may copy and modify the SDK example programs.

Liability. Pico Technology and its agents shall not be liable for any loss, damage or injury, howsoever caused, related to the use of Pico Technology equipment or software, unless excluded by statute.

Fitness for purpose. Because no two applications are the same, Pico Technology cannot guarantee that its equipment or software is suitable for a given application. It is your responsibility, therefore, to ensure that the product is suitable for your application.

Mission-critical applications. This software is intended for use on a computer that may be running other software products. For this reason, one of the conditions of the licence is that it excludes usage in mission-critical applications such as life-support systems.

Viruses. This software was continuously monitored for viruses during production, but you are responsible for virus-checking the software once it is installed.

Support. If you are dissatisfied with the performance of this software, please contact our technical support staff, who will try to fix the problem within a reasonable time. If you are still dissatisfied, please return the product and software to your supplier within 14 days of purchase for a full refund.

Upgrades. We provide upgrades, free of charge, from our web site at www.picotech.com. We reserve the right to charge for updates or replacements sent out on physical media.

2.7 Trademarks

Trademarks. Windows is a trademark of Microsoft Corporation in the United States and other countries. Pico Technology and PicoScope are internationally registered trademarks of Pico Technology Ltd.

Pico Technology and PicoScope are trademarks of Pico Technology Limited, registered in the United Kingdom and other countries.

PicoScope and Pico Technology are registered in the U.S. Patent and Trademark Office.

2.8 Warranty

Pico Technology warrants upon delivery, and for a period of 5 years from the date of delivery, that the Goods will be free from defects in material and workmanship.

Pico Technology shall not be liable for a breach of the warranty if the defect has been caused by fair wear and tear, wilful damage, negligence, abnormal working conditions or failure to follow Pico Technology's spoken or written advice on the storage, installation, commissioning, use or maintenance of the Goods or (if no advice has been given) good trade practice; or if the Customer alters or repairs such Goods without the written consent of Pico Technology.

2.9 Company details

Address: Pico Technology
James House
Colmworth Business Park
St. Neots
Cambridgeshire
PE19 8YP
United Kingdom

Phone: +44 (0) 1480 396 395

Fax: +44 (0) 1480 396 296

Email:

Technical Support: support@picotech.com

Sales: sales@picotech.com

Web site: www.picotech.com

3 Product information

3.1 Package contents

You can buy the PicoScope 6000 Series oscilloscopes with or without a set of 4 high-impedance 10:1 probes. Here are the contents of the 6 available product packs:

Code	Description	Product packs					
		PP628	PP629	PP630	PP631	PP748	PP749
-	PicoScope 6402	1	1				
-	PicoScope 6403			1	1		
-	PicoScope 6404					1	1
TA101*	500 MHz 10:1 compensated oscilloscope probes		4		4		
TA102	2-footed probe stand		1		1		1
TA133**	500 MHz 10:1 compensated oscilloscope probes						4
MI106	Hi-Speed USB cable	1	1	1	1	1	1
PS010	AC adapter	1	1	1	1	1	1
DI025	Software CD	1	1	1	1	1	1
DO115	USB Oscilloscope Installation Guide	1	1	1	1	1	1
MI251	Carry case	1	1	1	1	1	1

*350 MHz system bandwidth when used with PicoScope 6000 Series scopes.

**These 500 MHz probes are for the PicoScope 6404 only.

3.2 Minimum PC requirements

To ensure that your [PicoScope 6000 Series](#) oscilloscope operates correctly, you must have a computer with at least the minimum system requirements to run one of the supported operating systems, as shown in the following table. The performance of the software will increase with more powerful PCs, including those with multi-core processors.

Item	Specification
Operating system	Windows XP SP2 Windows Vista Windows 7
	32 bit and 64* bit versions supported
Processor	As required by Windows
Memory	
Free disk space	
Ports	USB 1.1 compliant port, or USB 2.0 compliant port (recommended)

* While the driver will run on a 64 bit operating system, the driver itself is 32 bit, and therefore will run as 32 bit.

3.3 Installation instructions

IMPORTANT

Always install the PicoScope software before connecting your [PicoScope 6000 Series](#) oscilloscope to the PC. This ensures that Windows will correctly recognize the oscilloscope.

Procedure

- Follow the instructions in the USB Oscilloscope Installation Guide included with your product package.
- Connect the AC adapter (supplied) to a power socket using the appropriate cable (also supplied), and connect the DC output of the AC adapter to the "DC Power" socket on the back of the oscilloscope.
- Connect the oscilloscope to the PC using the USB cable supplied.

Checking the installation

Once you have installed the software and connected the oscilloscope to the PC, start the [PicoScope](#) software. PicoScope should now display any signal connected to the scope inputs. If a probe is connected to your oscilloscope, you should see a small noise signal in the oscilloscope window when you touch the probe tip with your finger.

Moving the PicoScope PC Oscilloscope to another USB port

● Windows XP SP2

When you first installed the oscilloscope by plugging it into a [USB](#) port, Windows associated the Pico driver with that port. If you later move the oscilloscope to a different USB port, Windows will display the "New Hardware Found Wizard" again. When this occurs, just click "Next" in the wizard to repeat the installation. If Windows gives a warning about Windows Logo Testing, click "Continue Anyway". As all the software you need is already installed on your computer, there is no need to insert the Pico Software CD again.

● Windows Vista and Windows 7


The process is automatic. When you move the device from one port to another, Windows displays an "Installing device driver software" message and then a "PicoScope 6000 Series oscilloscope" message. The oscilloscope is then ready for use.

3.4 Connections

Standard oscilloscope connectors


The [PicoScope 6000 Series](#) oscilloscopes have standard BNC input and output connectors. The channel inputs have switchable impedances of 50 Ω or 1 M Ω . In high-impedance mode, they are compatible with all standard scope probes including 10:1 attenuated types. To ensure that you obtain the rated bandwidth from the scope, we recommend that you use the compensated high-frequency probes supplied with it.

Connector diagrams



Front panel
PicoScope 6000 Series

- A. [Input channel A](#)
- B. [Input channel B](#)
- C. [Input channel C](#)
- D. [Input channel D](#)
- E. [Probe calibration output](#)
- F. LED: shows when the oscilloscope is sampling data



Rear panel
PicoScope 6000 Series

- G. [DC power socket](#): for use with the AC adaptor supplied with the unit
- H. [USB 2.0 port](#): connects to your PC using the Hi-Speed USB cable supplied
- I. [SIGNAL OUT connector](#): carries the output of the arbitrary waveform generator and signal generator
- J. [AUX IN connector](#): carries the auxiliary (AUX) trigger and reference clock inputs
- K. Ventilation holes. Do not block the air intake holes or insert any objects through them, as this could damage the unit and cause injury.

3.5 Specifications

Model number	PicoScope 6402	PicoScope 6403	PicoScope 6404
Vertical section			
Number of channels	4		
Analog bandwidth ^[11]	350 MHz (-3 dB) with TA101 probe or direct 50 input		500 MHz (-3 dB) with TA133 probe or direct 50 input
Rise time (10%-90%)	1.0 ns		700 ps
Connectors	BNC female		
Input coupling ^[11]	AC 1 M , DC 1M , DC 50		
Input impedance	1 M (±1%) 15 pF or 50		1 M (±1%) 11 pF or 50
Voltage ranges ^[12] *1 M input only †250 MHz bandwidth	±50 mV†, ±100 mV, ±200 mV, ±500 mV, ±1 V, ±2 V, ±5 V, ±10 V*, ±20 V*		±50 mV, ±100 mV, ±200 mV, ±500 mV, ±1 V, ±2 V, ±5 V, ±10 V*, ±20 V*
Sensitivity (x1 zoom)	10 mV/div to 4 V/div		
Bandwidth limiter	Full or 20 MHz		Full or 25 MHz
Input offset (position) adjustment (1 M) range dependent	50 mV - 200 mV 500 mV - 2 V 5 V 10 V to 20 V	±0.5 V ±2.5 V ±20 V ±20 V	50 mV - 200 mV ±2 V 500 mV - 2 V ±10 V 5 V ±35 V 10 V ±30 V 20 V ±20 V
Input offset (position) adjustment (50) range dependent	50 mV - 200 mV 500 mV - 2 V 5 V	±0.5 V ±2.5 V ±0.5 V	50 mV - 200 mV ±2 V 500 mV ±5 V 1 V ±4.5 V 2 V ±3.5 V 5 V ±0.5 V
DC accuracy	3% of full scale		
Overload protection	±100 V DC+AC peak on 1 M inputs 5.5 V RMS on 50 inputs		
Acquisition			
Vertical resolution ^[11]	8 bits (up to 12 in resolution enhance mode)		
Maximum sampling rate ^[11] (real-time) One channel in use Two channels in use Three or four channels in use	5 GS/s 2.5 GS/s (when using the following channels AB, AC, BC, or BD) 1.25 GS/s		
Maximum streaming data rate	13 MS/s (PC-dependent)		
Buffer size ^[11]	32 MS ^[11]	1 GS ^[11]	
	shared between enabled channels		
Maximum buffer segments	32 k	1 M	
Timebase ranges ^[11]	1 ns/div to 200 s/div (real-time sampling)		
Timebase accuracy	5 ppm		
Triggering			
Trigger modes	Auto, repeat, none, rapid (segmented memory)		
Advanced digital triggers	Edge (rising/falling/dual) with adjustable hysteresis, Window, Pulse width, Window pulse width, Dropout, Window dropout, Interval, Logic, Runt pulse		
Trigger level	Adjustable over whole of selected voltage range		
Maximum trigger rate	Up to 10,000 waveforms in a 10 ms burst		
Re-arm time	Less than 1 μs on fastest timebase		
Trigger sources	Ch A to Ch D, AUX		
Maximum trigger delay	Pre-trigger: 100% of capture size Post-trigger: 4 billion samples		
Spectrum analyzer			
Frequency range	DC to 350 MHz		DC to 500 MHz
Display modes	Magnitude, average, peak hold		
Windowing functions	Rectangular, Gaussian, triangular, Blackman, Blackman-Harris, Hamming, Hann, flat-top		
Number of FFT points	Selectable from 128 to 1 million in powers of 2		

Probe calibration output		
Signal	1 kHz square wave, 2 V pk-pk, 600	
Overload protection	±5 V	
AUX input		
Connector	BNC female	
Impedance	50	
Coupling	DC	
Bandwidth (-3 dB)	25 MHz	
Threshold adjustment range	±1 V	
External clock input	Reference frequency 5 MHz to 25 MHz	
Protection range	±5 V	
Function generator and arbitrary waveform generator (AWG)		
Frequency range	DC to 20 MHz	
Standard waveforms	Sine, square, triangle, ramp, $\sin(x)/x$, Gaussian, half-sine, white noise, DC level, PRBS	
Amplitude flatness	3 dB	
DAC resolution	12 bits	
AWG sample rate	200 MS/s	
AWG buffer size	16,384 samples	
DC accuracy	1%	
Amplitude range	±250 mV to ±2 V	
Offset adjustment	±1 V (max. combined output ±2.5 V)	
Impedance	50	
Connector	BNC female	
Overload protection	±5 V	
Math channels		
Functions	-x, x+y, x-y, x*y, x/y, sqrt(x), x^y, exp(x), ln(x), log(x), abs(x), norm(x), sign(x), sin(x), cos(x), tan(x), arcsin(x), arccos(x), arctan(x), sinh(x), cosh(x), tanh(x), Pi	
Operands	A to D (input channels), T (time), reference waveforms, Pi	
Serial decoding		
Baud rate	10 kb/s to 1 Mb/s	
Threshold voltage	Adjustable	
Protocols	CAN Bus, I ² C, SPI, RS232, UART	
Mask limit testing		
Statistics	Pass/fail, failure count, total count	
Display		
Interpolation	Linear or $\sin(x)/x$	
Persistence modes	Digital color, analog intensity, custom, or none	
Environmental conditions		
Operating environment		
Temperature range	0 °C to 40 °C operational 20 °C to 30 °C for stated accuracy	
Humidity	5% to 80% RH, non-condensing	
Fan speed	Automatic, to reduce noise	
Storage environment		
Temperature range	-20 °C to +60 °C	
Humidity	5% to 95% RH, non-condensing	
IP rating	IP 20	
Miscellaneous		
PC connection	Hi-Speed USB 2.0	
Power supply	External AC to 12 V 3.5 A DC adapter and cables (cords) included	
Dimensions	170 mm x 255 mm x 40 mm (6.7" x 10.0" x 1.6") including connectors and plastic end caps	170 mm x 285 mm x 40 mm (6.7" x 11.2" x 1.6") including connectors and plastic end caps
Weight	< 1 kg (approx. 2 lb 3 oz)	1.3 kg (approx. 2 lb 14 oz)
Compliance	Europe: EMC EN61326, LVD EN61010-1, RoHS, WEEE USA: FCC Rules Part 15 Class A ³	
Languages supported	Full: English, French, Italian, German, Spanish User interface only: Chinese (Simplified and Traditional), Czech, Danish, Dutch, Finnish, Greek, Hungarian, Japanese, Norwegian, Polish, Portuguese, Romanian, Russian, Swedish and Turkish	

4 Glossary

Analog bandwidth. The input frequency at which the measured signal amplitude is 3 decibels below the true signal amplitude.

Buffer size. The size of the oscilloscope buffer memory, measured in samples. The buffer allows the oscilloscope to sample data faster than it can transfer it to the computer.

Coupling. To switch between AC coupling and DC coupling in PicoScope, select AC or DC from the control on the toolbar. The AC setting filters out very low-frequency components of the input signal, including DC, and is suitable for viewing small AC signals superimposed on a DC or slowly changing offset. In this mode you can measure the peak-to-peak amplitude of an AC signal but not its absolute value. Use the DC setting for measuring the absolute value of a signal.

Device Manager. Device Manager is a Windows program that displays the current hardware configuration of your computer. Right-click 'My Computer', select 'Manage' and then select 'Device Manager'.

Driver. A program that controls a piece of hardware. The driver for the oscilloscopes is supplied in the form of a 32-bit Windows DLL, `ps6000.dll`. This is used by the PicoScope software, and by user-designed applications, to control the oscilloscopes.

GS. Gigasamples (1,000,000,000 samples).

Maximum sampling rate. A figure indicating the maximum number of samples the oscilloscope can acquire per second. The higher the sampling rate of the oscilloscope, the more accurate the representation of the high-frequency details in a fast signal.

MS. Megasamples (1,000,000 samples).

PC Oscilloscope. A virtual instrument formed by connecting a PicoScope oscilloscope to a computer running the PicoScope software.


PicoScope 6000 Series. A range of 8-bit USB oscilloscopes from Pico Technology, with a sampling rate of 5 GS/s, bandwidths of 350 to 500 MHz and buffer sizes up to 1 GS.

PicoScope software. A software product that accompanies all PicoScope oscilloscopes. It turns your PC into an oscilloscope, spectrum analyzer and multimeter.

Timebase. The timebase controls the time interval that each horizontal division of a scope view represents. There are ten divisions across the scope view, so the total time across the view is ten times the timebase per division.

USB 2.0. Universal Serial Bus. This is a standard port used to connect external devices to PCs. The port supports a data transfer rate of up to 480 megabits per second, so is much faster than the RS-232 COM ports found on older PCs.

Vertical resolution. A value, in bits, indicating the precision with which the oscilloscope converts input voltages to digital values. [Oversampling](#)^[17] (see above) can improve the effective vertical resolution.

Voltage range. The range of input voltages that the oscilloscope can measure. For example, a voltage range of ± 100 mV means that the oscilloscope can measure voltages between -100 mV and +100 mV. Input voltages outside this range will not damage the instrument as long as they remain within the protection limits stated in the [Specifications](#)  table.

Index

A

- Accuracy 9
- Analog bandwidth 9

B

- Bandwidth (analog) 9
- BNC connector 8
- Buffer size 9

C

- Cable, USB 6
- Calibration output 8
- Carry case 6
- CD, software and reference 6
- CE notice 3
- Company information 5
- Compliance 9
- Connections 8
- Contact details 5

D

- Dimensions 9

E

- EMC Directive 3
- External trigger 8

F

- FCC notice 3

G

- Grounding 2

I

- Input range, maximum 9
- Inputs 9
- Installation 7

L

- LED 8
- Low Voltage Directive (LVD) 3

M

- Mains voltages 2

O

- Operating environment 9
- Oscilloscope probe 8
- Outputs 9
- Overload protection 9

P

- PC connection 9
- PC requirements 6
- Pico Technical Support 5
- PicoScope 6000 Series 1
- PicoScope software 7
- Power socket 8
- Power supply 9
- Probes, oscilloscope 6

R

- Resolution, vertical 9

S

- Safety
 - symbols 2
 - warning 2
- Sampling rate 9
- Scope probe 8
- Signal generator 9
 - output 8
- Software license conditions 4
- Specifications 9
- Storage environment 9

T

- Technical support 5
- Trademarks 5
- Trigger
 - bandwidth 9
 - external 8, 9

U

- USB 6
 - changing ports 7
- USB cable 6

V

Vertical resolution 9

Voltage ranges 9

W

Warning triangle 2

Warranty 5

Weight 9



Pico Technology

James House
Colmworth Business Park
ST. NEOTS
Cambridgeshire
PE19 8YP
United Kingdom
Tel: +44 (0) 1480 396 395
Fax: +44 (0) 1480 396 296
www.picotech.com

ps6000.en-2

27.05.11

Copyright © 2009-2011 Pico Technology Ltd. All rights reserved.